

NDIR GAS ANALYZER

DATA SHEET

ZPA

OVERVIEW

This gas analyzer (ZPA) can measure the concentration of NO, SO₂, CO₂, CO, CH₄ and O₂ in sample gas. NO, SO₂, CO₂, CO and CH₄ are measured by non-dispersion infrared method (NDIR), while O₂ is measured by a galvanic fuel cell, paramagnetic sensor, or zirconia sensor.

Up to five components including O₂ can be measured. ZPA also features its compact design that enables downsizing of measurement system, and simple structure with singlebeam IR system that requires minimal maintenance.

ZPA is best suited to the measurement of exhaust gas from refuse incinerators, boilers, and various industrial furnaces.

FEATURES

- 1. Compact and lightweight H133 × W483 × D382 mm, approximate 11 kg
- 2. Easy maintenance Maintenance is easy due to the simple measurement unit of single-beam system adapted.
- User-friendly operation Clear and easy-to-read display of all five gas concentrations at once.

Simple status and maintenance messages.

4. Extensive functions

Various optional functions are available such as auto calibration control, atmospheric pressure correction, high and low concentration alarms, remote range switch, and range identification signal,etc.

SPECIFICATIONS

Standard Specifications

Principle of measurement:

NO, SO₂, CO₂, CO, CH₄;

Non-dispersion infrared-ray absorption method Single light source and single beams (single beam system)

O2;

Galvanic fuel cell O_2 analyzer (built-in) paramagnetic O_2 analyzer (built-in), or zirconia O_2 analyzer (externally installed TYPE: ZFK7)

Measurable gas components and ranges:

	Minimum range	Maximum range
NO	0–200 ppm	0–5000 ppm
SO ₂	0–200 ppm	0–10 vol%
CO ₂	0–100 ppm	0–100 vol%
СО	0–200 ppm	0–100 vol%
CH ₄	0–500 ppm	0–100 vol%
O ₂ (Built in fuel cell)	0–10 vol%	0–25 vol%
O ₂ (Built in	0–5 vol%	0–100 vol%
paramagnetic)	None	100–95 vol%
O ₂ (External zirconia)	0–5 vol%	0–25 vol%



- Max. 5 components measurement including O₂. For reverse range O₂ measurement, infrared gas measurement is not available; only the single range O₂ measurement is available.
- Measuring ranges are changeable between the specified minimum and maximum range
- Maximum rangeability. 1:10 (except O₂)
- Up to two ranges are available for each component
- For possible combinations of components and ranges, refer to Table1.

Measured value indication:

Digital indication in 4 digits

- (LCD panel with LED back light)
- Instantaneous value of each component
- Instantaneous value after O2 correction
- (only in NO, SO₂, CO measurement with O₂)
- Average value after O2 correction
- (only in NO, SO₂, CO measurement with O₂)

O₂ average value

Analog output signals:

4 to 20mA DC or 0 to 1V DC, isolated internally from circuit and ground. Output lines are non-isolated each other.; 12 outputs max.

- Allowable load 550 Ω for 4 to 20mA DC
- Allowable load $100K\Omega$ for 0 to 1V DC
- * Refer to Table2 for the channel No. of displayed values and analog output signals.

Analog input signal:

- For signal input from external O2 analyzer.
- (1) Signal from Fuji's Zirconia O2 analyzer (TYPE: ZFK7)
- (2) 0 to 1V DC full-scale signal
- * Input section is not isolated.
- * External O₂ analyzer should be purchased separately.

Digital output (Option):

- 1 form C contact (24V DC/1A, resistive load) Up to 15 outputs
 - Instrument error, calibration error, range identification, auto calibration status, solenoid valve drive for auto calibration, high/low limit alarm
- * All relay contacts are isolated mutually and from the internal circuit.

Digital input (Option):

Voltage contact (12-24V DC, ≤15mA) Up to 9 inputs

Remote range change over, auto calibration remote start, remote hold, average value reset.

* Isolated from the internal circuit with photocoupler.

Power supply:

Voltage rating; 100V to 240V AC Allowable range: 85V to 264V AC

Frequency; 50Hz/60Hz

Power consumption; 100VA max.

Operating conditions:

Ambient temperature; -5°C to 45°C

(40°C max. when using two optical systems with 200V AC power source)

Ambient humidity; 90% RH max., non-condensing

Storage conditions:

Ambient temperature; -20°C to 60°C

Ambient humidity; 95% RH max., non-condensing **Dimensions (H × W × D):** 133 × 483 × 382mm

Weight: Approx. 11 kg

Finish color: Front panel; Cool gray (PANTON 1C-F) Enclosure:

Steel casing, for indoor use

Material of gas-contacting parts:

Gas inlet/outlet; Stainless steel 304

Sample cell; Stainless steel 304,chloroprene rubber Infrared-ray transmitting window; CaF2 Internal piping; vinyl chloride, PTFE, Polypropylene Paramagnetic O₂ analyzer cell: Stainless steel 316

Fuel cell O₂ analyzer cell: ABS resin Gas inlet/outlet: Rc1/4 or NPT1/4 internal thread

Purge gas flow rate: 1L/min (when required)

Life time of galvanic fuel cell O2 analyzer: 2 years

Standard Functions

Output signal holding:

Enables you to hold the output signal during calibration, to the value right before the calibration is started or the user-specified value. Values indicated on LCD will not be held.

Range changeover:

You can change between ranges by manually, automatically, or remotely.

Manual: by key operation

Auto: When the measured value reaches above 90% FS of the 1st range, the range automatically switches to the 2nd range. When the measured value goes down below 80% FS of the 1st range, the range automatically switches from the 2nd range to the 1st range.

Remote: by the contact input (option).

When the specified voltage (the remote range changeover signal) is applied on the contact dedicated for each component, the 1st range is effective. When no voltage is applied, the 2nd range becomes effective.

Optional Functions

Remote output holding:

Applying the specified voltage on the dedicated terminal allows you to hold the output signal to the last value or the user-specified value. Holding is effective while the voltage is applied. Values indicated on LCD are not held. **Range identification signal:**

You can check which range is in use.

Auto calibration:

This function requires standard gas cylinders for calibration and solenoid valves for opening/closing the gas flow line. When this function is activated, the analyzer opens and closes the solenoid valve driving contact periodically at preset cycle.

Auto calibration cycle setting:

1 hour to 99 hours (in increments of 1 hour) or

1 day to 40 days (in increments of 1 day).

Gas flow time setting:

The time during which calibration gas is drawn

60 seconds to 900 seconds (in increments of 1 second) Auto calibration remote start:

When you apply the specified voltage for 1.5 seconds or longer on the auto calibration remote start contact and then open the contact, one-time auto calibration starts. Calibration gas is drawn for the time set in the "gas flow time setting" for Auto calibration (see the previous item).

Auto zero calibration:

This function requires a standard gas cylinder for zero calibration and a solenoid valve for opening/closing the gas flow line. When this function is activated, the analyzer opens and closes the solenoid valve driving contact periodically at preset cycle. The cycle for the auto zero calibration and that for the auto calibration can be different. Auto calibration cycle setting:

1 hour to 99 hours (in increments of 1 hour) or

1 day to 40 days (in increments of 1 day).

Gas flow time setting:

The time during which calibration gas is drawn

60 seconds to 900 seconds (in increments of 1 second) Upper/lower limit alarm:

When an instantaneous value has gone beyond the upper limit or below the lower limit, the analyzer closes the contact to emit an alarm signal. Up to four alarms are available.

Instrument error contact output:

The contact is closed if a device error occurs.

Calibration error contact output:

The contact is closed if a calibration error occurs.

Auto calibration status contact output:

The contact is closed during auto calibration.

O₂ correction:

Conversion of measured NO, CO, and SO₂ gas concentrations into values at reference O₂ concentration Correction formula:

$$C = \frac{21-On}{21-Os} \times Cs$$

C: Sample gas concentration after O₂ correction Cs: Measured concentration of sample gas

Os: Measured O_2 concentration

On: Reference O_2 concentration

(changeable by setting)

* The upper limit value of the fractional part in this calculation is 4. The result of calculation is indicated and transmitted as an analog output signal.

Average value after O_2 correction and O_2 average value calculation:

The analyzer can take measurement every 30 seconds, and calculate the moving average of instantaneous concentration after O_2 correction or instantaneous O_2 value per the period you set; in the range 1–59 min (in one minute increment) or 1–4 hour (in one hour increment). The analyzer transmits the moving average output every 30 seconds.

Average value resetting:

The above-mentioned output of average value is started from the initial state by opening the average value resetting input terminals after short circuiting for 1.5 sec or longer. Output is reset by input voltage and restarted by opening the terminal circuit.

Communication function:

RS-485 (9pins D-sub connector) Half-duplex bit serial Start-stop synchronization Modbus RTU[™] protocol

Contents: Read/Write parameters

Read measurement concentration and instrument status

When connecting via RS-232C interface, an RS-232C \leftrightarrow RS-485 converter should be used.

Atmospheric pressure correction:

Measure atmospheric pressure and calculate compensation (for use, be sure to relieve the exhaust gas from analyzer to the atmosphere)

After atmospheric pressure correction;

- Zero point: No influenced
- Span point: The change is 0.5% measured value or less relating to the change of the atmospheric pressure 1%.

Correction range: 700hPa-1050hPa

Performance

Repeatability: ±0.5% of full scale

Linearity:

1% of full scale

prior to atmospheric pressure correction (option) Zero drift:

±2% of full scale/week

In the case of NO and/or SO₂ measurement below 500 ppm range, with the auto zero calibration used.

Span drift: ±2% of full scale/week

Response time (for 90% FS response) :

1 to 15 sec electrical response. Within 10-30 seconds including replacement time of sampling gas.

Gas replacement time depends on the number of measuring components, and measuring range.

Interference from other gases:

Interference component	CO ₂ measurement	CO measurement	CH ₄ measurement	SO ₂ measurement	NO measurement	O2 measurement (built-in paramagnetic)
CO 1000 ppm	≤ 1.0% FS	-	≤ 1.0% FS	≤ 1.0% FS	≤ 1.0% FS	-
CO2 15%	-	≤ 1.0% FS ^{*1}	≤ 1.0% FS	≤ 1.0% FS	≤ 1.0% FS ^{*2}	≤ 2.0% FS
H ₂ O saturation at 20°C	≤ 1.0% FS	≤ 1.0% FS ^{*3}	≤ 1.0% FS ^{*4}	-	-	-
H ₂ O saturation at 2°C	-	≤ 2.0% FS	≤ 1.0% FS ^{*5}	≤ 2.0% FS	≤ 2.0 % FS	≤ 1.0vol% O ₂
CH4 1000 ppm	≤ 1.0% FS	≤ 1.0% FS	-	≤ 20 ppm	-	-
		-				

1: 0-200 ppm range: ≤ 2.0% FS

*2: Less than 0-500ppm renge: ≤ 2.0%FS
*3: 0-500 ppm range: ≤ 2.0% FS Not applicable for less than 0-500ppm range
*4: Not applicable for less than 0-5000ppm range

*5: Below 0-5000 ppm range

Requirements for Sample Gas

Flow rate: 0.5 ±0.2L / min

Temperature: 0 to 50°C

Pressure:

10 kPa or less (Gas outlet side should be open to the atmospheric air.)

Dust:

100 µg/Nm³ or less in particle size of 0.3 µm or smaller Mist: Unallowable

Moisture:

- Less than standard room temperature dew point. (No condensation)
- However, 2°C dew point or less for the following specifications.

Measurement of 0-200ppm CO, NO, SO₂, less than 0-5000ppm CH₄ and paramagnetic O₂.

Corrosive component:

1 ppm or less

Standard gas for calibration:

- 1) For measurement with IR and/or built-in O2 sensor Zero gas; Dry N₂
 - Span gas; Each sample gas having concentration of 90 to 100% of its measuring range (recommended).
- 2) For measurement with external zirconia O₂ sensor and when calibration is carried out on the same calibration gas line:
 - Zero gas; Dry air or atmospheric air (This is not allowed for CO₂ measurement.)
 - Span gas; For other than O₂ measurement, each sample gas having concentration of 90 to 100% of its measuring range
 - * For O₂ measurement, 1-2 vol% O₂, balance N₂
- 3) Reverse range O2 measurement

Zero gas; 100vol% O2

- Span gas; 95.0 to 95.5 vol% O₂, balance N₂
- * If you use the reverse range O2 measurement, IR measurement is not available.

Installation Requirements

- · Indoor use. Select a place where the equipment does not receive direct sunlight, wind and rain, or radiation from hot substances. If such a place cannot be found, a roof or cover should be prepared for protection.
- Avoid a place where unit receives heavy vibration
- · Select a place where atmospheric air is clean


EU Directive Compliance

•
CE
LVD (2014/35/EU)
EN 61010-1
EN 61010-2-030
EN 62311
EMC (2014/30/EU)
EN 61326-1 (Table 2)
EN 55011 (Group 1 Class A)
EN 61000-3-2 (Class A)
EN 61000-3-3
EN 61326-2-3
RoHS (2011/65/EU+(EU)2015/863)
EN IEC63000
UK CA
LVD (S.I.2016 No.1101)
EN 61010-1
EN 61010-2-030
EN 62311
EMC (S.I.2016 No.1091)
EN 61326-1 (Table 2)
EN 55011 (Group 1 Class A)
EN 61000-3-2 (Class A)
EN 61000-3-3
EN 61326-2-3
RoHS (S.I.2012 No.3032)


EN IEC 63000

PRINCIPLE


NDIR sensor (for CO₂, CO, CH₄, SO₂, NO)

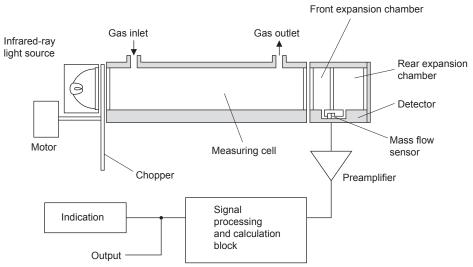

Paramagnetic sensor (for O₂)

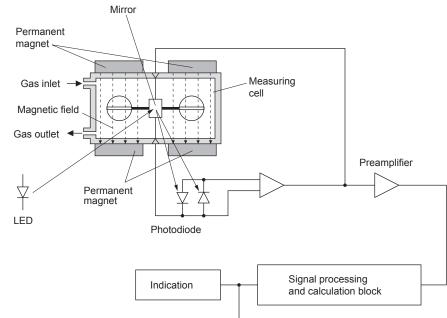


Galvanic fule cell (for O₂)

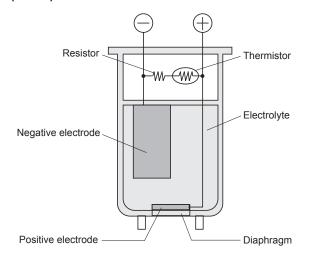


SYSTEM CONFIGURATION EXAMPLES

Example of not dehumidifying the moisture in the measurement gas.

Low moisture appreciation.

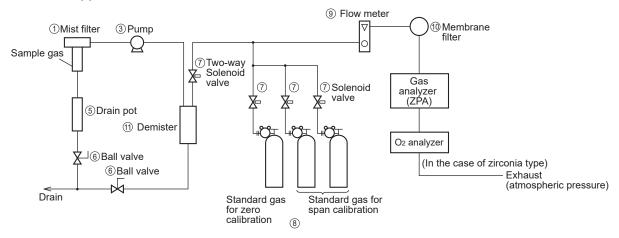

Example of dehumidifying the moisture in the measurement gas.

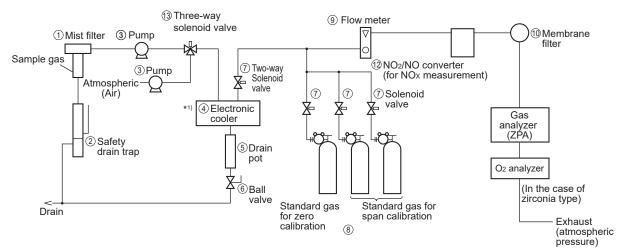

*1) For NO, SO₂, or 0–200 ppm range CO measurement, be sure to use an electronic cooler to keep the moisture content below the level saturated at 2°C.

List of sampling devices (example)

No.	Device name	Fuji's type
1	Mist filter	ZBBK1V03-0
2	Safety drain trap	ZBH51603
3	Pump	ZBG80
4	Electoric cooler	ZBC91004
(5)	Drain pot	ZBH13003 (Length 255mm)
6	Ball valve	ZBFB1
$\overline{\mathcal{O}}$	Two-way solenoid valve	
8	Standard gas for calibration	ZBM Y04-0 (Codes in to be selected depending on application)
9	Flow meter	ZBD42203
10	Membrane filter	ZBBM2V03-0
(11)	Demister	ZBH35003
12	NO ₂ /NO converter	ZDL02001
13	Three-way solenoid valve	

Note) The above is a typical configuration example. As configuration may differ depending on measuring objects, please consult us.

CODE SYMBOLS

		-				1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 1920 21 22 23 24 25 26 - D
Digit	Description				note	
4	<specification< td=""><td>n/Structure> e (Terminal bloc</td><td>k for power sur</td><td>ndv)</td><td></td><td></td></specification<>	n/Structure> e (Terminal bloc	k for power sur	ndv)		
	Horizontal tvn	e (Power inlet, v	vith lock)	עיקי)	note1	
5	<mounting></mounting>		,			
<u> </u>	19inch rack m	nounting type El/	A conformity			В
6		component (ND 2nd component		4th component		
	None	-	-	-	note2	2 Y
	NO	-	-	-		P
	SO ₂	-	-	-		
	CO ₂ CO	-	-	-		В
	CO CH₄	-	-	-		
	NO	SO ₂			1	- - + - + - + - + - + - + - + - + - + -
	NO	со	-	-		G
	SO ₂		-	-		
	CO2 CH4	CO CO	-	-		
		CH₄	-	-		
	NO	SO ₂	co	-	1	N
	CO ₂	со	CH4	-		
	NO Others	SO ₂	CO ₂	CO		
7		component (O2)	>			
'	None	,				
	External O ₂ a		(note3	3 1 1
1		nia O2 analyzer				
		nic fuel cell O₂ ar agnetic O₂ anal		eatment)	note12	2 4
1				nmental measurement)		
8	<revision cod<="" td=""><td>de></td><td></td><td></td><td></td><td>2</td></revision>	de>				2
9		ange (NDIR)>1s			note4	
10		ange (NDIR)>1s ange (NDIR)>2n			note4 note4	
11		ange (NDIR)>21			note4	
13		ange (NDIR)>3r			note4	
14	<measuring ra<="" td=""><td>ange (NDIR)>3r</td><td>d component, 2</td><td>nd range</td><td>note4</td><td></td></measuring>	ange (NDIR)>3r	d component, 2	nd range	note4	
15		ange (NDIR)>4th			note4	
16	<measuring ra<="" td=""><td>ange (NDIR)>4th ange (O₂)></td><td>n component, 2</td><td>nd range</td><td>note4 note4</td><td></td></measuring>	ange (NDIR)>4th ange (O ₂)>	n component, 2	nd range	note4 note4	
	None				110104	
	0-5/10vol%					
	0-5/25vol%					B
	0-10/25vol% 0-5vol%					
	0-10vol%					
	0-25vol%					V
	0-50vol%					P
	0-100vol% 100-95vol%					
	Others					S S S S S S S S S S S S S S S S S S S
18	<gas connect<="" td=""><td>tion></td><td></td><td></td><td>1</td><td></td></gas>	tion>			1	
	Rc1/4					
	NPT1/4 <output></output>					2
19	<output> 0–1V DC</output>					
	4–20mA DC					B
	0-1V DC + C	ommunication				c
		Communication			n=1 - 5	
20	<indication po<="" td=""><td>ower supply cord</td><td>l> 125V (PSE)</td><td></td><td>note5</td><td></td></indication>	ower supply cord	l> 125V (PSE)		note5	
	English, cord		125V (FSL) 125V (UL)			
	English, cord	rated	250V (CEE)			
	Chinese, cord		250V (CCC)	nut>	n=1 - 0	
21	<o2 correction<="" td=""><td>and O₂ correcti</td><td>on average out</td><td>pul></td><td>note6</td><td></td></o2>	and O ₂ correcti	on average out	pul>	note6	
	O ₂ correction					
	O ₂ correction average					B
	O ₂ correction and O ₂ correction average 2 <optional (dio)="" function=""></optional>					
22		ction (DIO)> Cal. H/L Alarm	RangelD/D	emote range	note7	
1	None	Jai. FI/L Alarm		smole range	·	
1						
1						B
1		0				
1		<u> </u>				<u>D</u>
1		\sim 1 \bigcirc	1		1	
						F
						F G

			1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21 22 23 24 25 25 -	🗕 Digit
Digit	Description	note		
23	<pressure compensation=""></pressure>			
	None		Y	
	Pressure compensation		1	
24	<unit></unit>			
	ppm, vol%		A	
	mg/m³, g/m³	note8	B	
25	<adjustment></adjustment>	note9		
	For standard		A	
	For heat treatment furnace	note10	C	
	For converter		D	
	Others		Z	
26	<others></others>			
	Non-standard		Z	

NDIR range codes

Range	Code	Range	Code
None	Y	0 to 1vol%	J
0 to 100ppm	В	0 to 2vol%	K
0 to 200ppm	C	0 to 3vol%	0
0 to 250ppm	D	0 to 5vol%	L
0 to 300ppm	S	0 to 10vol%	M
0 to 500ppm	E	0 to 20vol%	N
0 to 1000ppm	F	0 to 25vol%	V
0 to 2000ppm	G	0 to 40vol%	W
0 to 2500ppm	U	0 to 50vol%	P
0 to 3000ppm	Т	0 to 70vol%	X
0 to 5000ppm	н	0 to 100vol%	R
		Others	Z

O₂ range codes

Measurement range	Range code	Galvanic fuel cell (built - in)	Paramagnetic cell (built - in)	Zirconia cell (external)
0 to 5/10 vol%	А		O note11	0
0 to 5/25 vol%	В		O note11	0
0 to 10/25 vol%	С	0	0	0
0 to 5 vol%	L		⊖ note11	0
0 to 10 vol%	Μ	0	0	0
0 to 25 vol%	V	0	0	0
0 to 50 vol%	Р		0	
0 to 100 vol%	R		0	
100 to 95 vol%	S		0	

note1) If you select "D" in the 4th code, the analyzer comes with the power cable. Specify the rating of the power cable in the 20th code.

note2) If you use this analyzer only for oxygen measurement, select "Y" in the 6th code.

note3) If you use an external O₂ sensor (7th code "1"), set 0–1 V DC linear signals from the external O₂ analyzer so that they corresponds to the full scale setting of the analyzer. Note that the external O₂ analyzer (7th code"1") and the external zirconia O₂ sensor ZFK7 (7th code "2") need to

Note that the external O_2 analyzer (/th code"1") and the external zirconia O_2 sensor ZFK7 (/th code "2") need to be ordered separately.

note4) Check the possible combination of measuring components and ranges in Table 1. Specify the range with the range codes shown in the above tables.

note5) If you select "D" in the 4th code, select the appropriate cable specification for end user in the 20th code. If you select "A" in the 4th code, the power cable is not supplied. If you need no power cable and want to order the manual written in English, select "E" in the 20th code.

note6) O₂ correction is provided only for NO, SO₂, and CO measurement.

When "H" is specified for the 6th digit, "A, B, or C" cannot be selected for the 21st digit.

note7) The 22nd code "H" is not available for five-component measurement. If you use four-component measurement and select "H" in the 22nd code, the maximum number of the H/L alarm outputs is three.

note8) Even if you selected "B" in the 24th code, select the range in ppm that is shown in the above "NDIR range codes" table. We will set the analyzer after converting the ppm ranges into mg/m³ ranges. For the converted ranges, see the "ppm-mg/m³ conversion table" shown below.

note9) When A, C, or D is specified at 25th digit, the analyzer will be adjusted and delivered with the following balance gasses. Standard "A": balance gas N₂

For heat treatment furnace "C": CO₂ analyzer: 25% CO + 30% H₂ + residue N₂

CO analyzer: 5% CO₂ + 30% H₂ + residue N₂

CH₄ analyzer: 25% CO + 30% H₂ + residue N₂

For converter "D": balance gas CO, CO

When other adjustment is required, please select "Z". In that case, please provide a list of gas composition of the process gas.

note10) When the 25th code is "C", the range codes "X" and "R" are not available.

- note11) NDIR range codes "V", "W", "P", "X", and "R" are not available.
- note12) When the hydrogen concentration in sample gas is 1% or more, select "4."

Demana anda	0.0.00	Range in mg/m ³			
Range code	ppm	NO	SO ₂	CO	
С	0–200	—	_	0–250 mg/m ³	
D	0–250	—	_	0–300 mg/m ³	1
S	0–300	—	—	0–375 mg/m ³	
E	0–500	0–650 mg/m ³	0–1400 mg/m ³	0–600 mg/m ³	
F	0–1000	0–1300 mg/m ³	0–2800 mg/m ³	0–1250 mg/m ³	
G	0–2000	0–2600 mg/m ³	0–5600 mg/m ³	0–2500 mg/m ³	Co
U	0–2500	0–3300 mg/m ³	0–7100 mg/m ³	0–3000 mg/m ³	NC
Т	0–3000	0–4000 mg/m ³	0–8500 mg/m ³	0–3750 mg/m ³	sc
Н	0–5000	0–6600 mg/m ³	0–14.00 g/m ³	0-6250 mg/m ³] cc

ppm-mg/m³ conversion table

Conversion formula NO (mg/m³) = 1.34 × NO (ppm) SO₂ (mg/m³) = 2.86 × SO₂ (ppm) CO (mg/m³) = 1.25 × CO (ppm)

Table 1 Measurable component and range - availability check table -

Range selection procedure

One component analyzer:

First determine 1st range, then select 2nd range from the corresponding column.

Two or more component analyzer:

- 1. Check the available options referring to the below tables, and determine the 1st range. Select the corresponding range code from "NDIR range codes" on Page 8.
- 2. The 2nd range must be greater than the 1st range but no greater than the value in the column "2nd range (max.)". Check the available options referring to the below tables, and determine the 2nd range. Select the corresponding range code from "NDIR range codes" on Page 8.

1-component analyzer : CO

1st range	2nd range
0 - 200ppm	None, 0 - 250ppm,300ppm,500ppm,1000ppm,2000ppm
0 - 250ppm	None, 0 - 300ppm,500ppm,1000ppm,2000ppm,2500ppm
0 - 300ppm	None, 0 - 500ppm,1000ppm,2000ppm,2500ppm
0 - 500ppm	None, 0 - 1000ppm,2000ppm,2500ppm,3000ppm,5000ppm
0 - 1000ppm	None, 0 - 2000ppm,2500ppm,3000ppm,5000ppm,1%
0 - 2000ppm	None, 0 - 2500ppm,3000ppm,5000ppm,1%,2%
0 - 2500ppm	None, 0 - 3000ppm,5000ppm,1%,2%
0 - 3000ppm	None, 0 - 5000ppm,1%,2%
0 - 5000ppm	None, 0 - 1%,2%,3%,5%
0 - 1%	None, 0 - 2%,3%,5%,10%
0 - 2%	None, 0 - 3%,5%,10%,20%
0 - 3%	None, 0 - 5%,10%,20%,25%
0 - 5%	None, 0 - 10%,20%,25%,40%,50%
0 - 10%	None, 0 - 20%,25%,40%,50%,70%,100%
0 - 20%	None, 0 - 25%,40%,50%,70%,100%
0 - 25%	None, 0 - 40%,50%,70%,100%
0 - 40%	None, 0 - 50%,70%,100%
0 - 50%	None, 0 - 70%,100%
0 - 70%	None, 0 - 100%
0 - 100%	None

1-component analyzer : CO2

1st range	2nd range
0 - 100ppm	None, 0 - 200ppm,250ppm,300ppm,500ppm,1000ppm
0 - 200ppm	None, 0 - 250ppm,300ppm,500ppm,1000ppm,2000ppm
0 - 250ppm	None, 0 - 300ppm,500ppm,1000ppm,2000ppm,2500ppm
0 - 300ppm	None, 0 - 500ppm,1000ppm,2000ppm,2500ppm
0 - 500ppm	None, 0 - 1000ppm,2000ppm,2500ppm,3000ppm,5000ppm
0 - 1000ppm	None, 0 - 2000ppm,2500ppm,3000ppm,5000ppm,1%
0 - 2000ppm	None, 0 - 2500ppm,3000ppm,5000ppm,1%,2%
0 - 2500ppm	None, 0 - 3000ppm,5000ppm,1%,2%
0 - 3000ppm	None, 0 - 5000ppm,1%,2%
0 - 5000ppm	None, 0 - 1%,2%,3%,5%
0 - 1%	None, 0 - 2%,3%,5%,10%
0 - 2%	None, 0 - 3%,5%,10%,20%
0 - 3%	None, 0 - 5%,10%,20%,25%
0 - 5%	None, 0 - 10%,20%,25%,40%,50%
0 - 10%	None, 0 - 20%,25%,40%,50%,70%,100%
0 - 20%	None, 0 - 25%,40%,50%,70%,100%
0 - 25%	None, 0 - 40%,50%,70%,100%
0 - 40%	None, 0 - 50%,70%,100%
0 - 50%	None, 0 - 70%,100%
0 - 70%	None, 0 - 100%
0 - 100%	None

1-compone	nt analyzer : NO
1st range	2nd range
0 - 200ppm	None, 0 - 250ppm,300ppm,500ppm,1000ppm,2000ppm
0 - 250ppm	None, 0 - 300ppm,500ppm,1000ppm,2000ppm,2500ppm
0 - 300ppm	None, 0 - 500ppm,1000ppm,2000ppm,2500ppm
0 - 500ppm	None, 0 - 1000ppm,2000ppm,2500ppm,3000ppm,5000ppm
0 - 1000ppm	None, 0 - 2000ppm,2500ppm,3000ppm,5000ppm
0 - 2000ppm	None, 0 - 2500ppm,3000ppm,5000ppm
0 - 2500ppm	None, 0 - 3000ppm,5000ppm
0 - 3000ppm	None, 0 - 5000ppm
0 - 5000ppm	None
1-compone	nt analyzer : SO2
1st range	2nd range
0 - 200ppm	None, 0 - 250ppm,300ppm,500ppm,1000ppm,2000ppm
0 - 250ppm	None, 0 - 300ppm,500ppm,1000ppm,2000ppm,2500ppm
0 - 300ppm	None, 0 - 500ppm,1000ppm,2000ppm,2500ppm
0 - 500ppm	None, 0 - 1000ppm,2000ppm,2500ppm,3000ppm,5000ppm
0 - 1000ppm	None, 0 - 2000ppm,2500ppm,3000ppm,5000ppm,1%
0 - 2000ppm	None, 0 - 2500ppm,3000ppm,5000ppm,1%,2%
0 - 2500ppm	None, 0 - 3000ppm,5000ppm,1%,2%
0 - 3000ppm	None, 0 - 5000ppm,1%,2%
0 - 5000ppm	None, 0 - 1%,2%,3%,5%
0 - 1%	None, 0 - 2%,3%,5%,10%
0 - 2%	None, 0 - 3%,5%,10%
0 - 3%	None, 0 - 10%
0 - 5%	None, 0 - 10%
0 - 10%	None
1-compone	nt analyzer : CH4
1st range	2nd range
0 - 500ppm	None, 0 - 1000ppm,2000ppm,2500ppm,3000ppm,5000ppm
0 - 1000ppm	None, 0 - 2000ppm,2500ppm,3000ppm,5000ppm,1%
0 - 2000ppm	None, 0 - 2500ppm,3000ppm,5000ppm,1%,2%
0 - 2500ppm	None, 0 - 3000ppm,5000ppm,1%,2%
0 - 3000ppm	None, 0 - 5000ppm,1%,2%
0 - 5000ppm	None, 0 - 1%,2%,3%,5%
0 40/	N 0.00% 00% F0% 400%

 0 - 1%
 None, 0 - 2%,3%,5%,10%

 0 - 2%
 None, 0 - 3%,5%,10%,20%

 0 - 3%
 None, 0 - 5%,10%,20%,25%

 0 - 5%
 None, 0 - 10%,20%,25%,40%,50%

 0 - 10%
 None, 0 - 20%,25%,40%,50%,70%,100%

 0 - 20%
 None, 0 - 25%,40%,50%,70%,100%

 0 - 25%
 None, 0 - 25%,40%,50%,70%,100%

 0 - 40%
 None, 0 - 50%,70%,100%

 0 - 50%
 None, 0 - 50%,70%,100%

 0 - 50%
 None, 0 - 70%,100%

 0 - 70%
 None, 0 - 100%

 0 - 100%
 None

2-component analyzer : NO/SO2

1-componen	t : NO		2-component : SO ₂				
1st range	2nd range (max.)		1st range	2nd range (max.)			
0 - 200ppm	0 - 2000ppm	(0 - 200ppm	0 - 2000ppm			
0 - 250ppm	0 - 2500ppm		0 - 250ppm	0 - 2500ppm			
0 - 300ppm	0 - 2500ppm	Select the second component from	0 - 300ppm	0 - 2500ppm			
0 - 500ppm	0 - 5000ppm	the table on the right.	0 - 500ppm	0 - 5000ppm			
0 - 1000ppm	0 - 5000ppm	l →	0 - 1000ppm	0 - 5000ppm			
0 - 2000ppm	0 - 5000ppm		0 - 2000ppm	0 - 5000ppm			
0 - 2500ppm	0 - 5000ppm		0 - 2500ppm	0 - 5000ppm			
0 - 3000ppm	0 - 5000ppm		0 - 3000ppm	0 - 5000ppm			
0 - 5000ppm	None] (0 - 5000ppm	None			

2-component analyzer : NO/CO

1-component	t · NO		2-component : CO		
•	1	-			
1st range	2nd range (max.)		1st range	2nd range (max.)	
0 - 200ppm	0 - 2000ppm		0 - 200ppm	0 - 2000ppm	
0 - 250ppm	0 - 2500ppm		0 - 250ppm	0 - 2500ppm	
0 - 300ppm	0 - 2500ppm	Select the second component from	0 - 300ppm	0 - 2500ppm	
0 - 500ppm	0 - 5000ppm	the table on the right.	0 - 500ppm	0 - 5000ppm	
0 - 1000ppm	0 - 5000ppm] … →<	0 - 1000ppm	0 - 5000ppm	
0 - 2000ppm	0 - 5000ppm		0 - 2000ppm	0 - 5000ppm	
0 - 2500ppm	0 - 5000ppm		0 - 2500ppm	0 - 5000ppm	
0 - 3000ppm	0 - 5000ppm		0 - 3000ppm	0 - 5000ppm	
0 - 5000ppm	None		0 - 5000ppm	None	

2-component analyzer : SO₂/CO₂

2-component analyzer : 502/C02						
1-componen	t : SO2	Select the second	2-component : CO2			
1st range	2nd range (max.)	component from the table on the	1st range	2nd range (max.)		
0 - 200ppm	0 - 2000ppm	right.	0 - 10%	0 - 25%		
0 - 250ppm	0 - 2500ppm					
0 - 300ppm	0 - 2500ppm					
0 - 500ppm	0 - 5000ppm					
0 - 1000ppm	0 - 5000ppm					
0 - 2000ppm	0 - 5000ppm					
0 - 2500ppm	0 - 5000ppm					
0 - 3000ppm	0 - 5000ppm					
0 - 5000ppm	None					

2-component analyzer: CO₂/CO

2-componen	t analyzer: CO	2/CO
1-componen	t: CO2	2-component: CO
1st range	2nd range (max.)	1st range/2nd range (max.)
0-100ppm	0-1000ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/2500ppm, 0-1000/2500ppm, 0-2000/2500ppm, 0-2500ppm
0-200ppm	0-2000ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/5000ppm, 0-1000/5000ppm, 0-2000/5000ppm, 0-2500/5000ppm
0-250ppm	0-2500ppm	0-3000ppm/2%, 0-5000ppm/3%, 0-1/3%, 0-2/3%, 0-3%
0-300ppm		
0-500ppm		
0-500ppm	0-5000ppm	0-500/5000ppm, 0-1000/5000ppm, 0-2000/5000ppm, 0-2500/5000ppm, 0-3000ppm/2%, 0-5000ppm/3%, 0-1/3%, 0-2/3%, 0-3%
0-1000ppm	0-5000ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%,
0-2000ppm	0-5000000000000000000000000000000000000	0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/10%, 0-3/10%, 0-5/50%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%
	0-1%	
0-1000ppm		0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/10%, 0-3/10%, 0-5/50%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-2000ppm	0-1%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/10%, 0-3/25%, 0-5/50%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-2000ppm	0-2%	0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/10%, 0-3/25%, 0-5/50%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-2500ppm	0-1%	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/10%, 0-3/25%, 0-5/50%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-2500ppm	0-2%	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/10%, 0-3/25%, 0-5/50%, 0-10/50%, 0-25/50%, 0-40/50%, 0-50%
0.2000	0.10/	
0-3000ppm	0-1%	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/10%, 0-3/25%, 0-5/50%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-3000ppm	0-2%	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/10%, 0-3/25%, 0-5/25%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-5000ppm	0-3%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%,
0-1%	0-5%	0-3/25%, 0-5/50%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-2%	0-5%	
0-5000ppm	0-5%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/50%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-1%	0-10%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%,
U 1/0		0-3/25%, 0-5/25%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-2%	0-20%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%,
0-2/0	0-20 /0	0-3/25%, 0-5/50%, 0-10/50%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-2%	0-10%	0-5/25%, 0-5/50%, 0-10/50%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100% 0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%,
0-2%	0-10%	0-3/25%, 0-5/50%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-3%	0-25%	0-3/25 /6, 0-3/30 /6, 0-10/100 /6, 0-20/100 /6, 0-25/100 /6, 0-40/100 /6, 0-50/100 /6, 0-70/100 /6, 0-100/0
		0.1000ppp=19/.0.2000ppp=19/.0.2500ppp=19/.0.2000pp=-20/.0.5000p=
0-10%	0-100%	0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%,
0-20%		0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-25%		
0-40%		
0-50%		
0-70%		
0-100%	None	

2-component analyzer: CH4/CO

	nt analyzer: CH	
1-componen		2-component: CO
1st range		1st range/2nd range (max.)
0-500ppm	0-5000ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/2500ppm, 0-1000/2500ppm, 0-2000/2500ppm
0-1000ppm		0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/5000ppm, 0-1000/5000ppm, 0-2000/5000ppm, 0-2500/5000ppm, 0-3000/5000ppm
0-1000ppm	0-1%	0-500/5000ppm, 0-1000/5000ppm, 0-2000/5000ppm, 0-2500/5000ppm, 0-3000/5000ppm
0-2000ppm	0-5000ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%
0-2500ppm	0-5000ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1% 0-3000ppm/1%,
0-3000ppm	1	0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/25%, 0-5/25%, 0-10/25%
0-2000ppm	0-1%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%
0-2500ppm	0-1%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/25%, 0-5/25%, 0-10/25%
0-3000ppm		
0-2000ppm	0-2%	0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%
0-2500ppm		0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/25%, 0-5/25%, 0-10/25%
0-3000ppm		
0-5000ppm	0-1%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/20%,
		0-3/25%, 0-5/50%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-5000ppm	0-3%	0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/10%, 0-3/25%, 0-5/50%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-5000ppm		0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/5%, 0-3/25%, 0-5/25%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-1%	0-5%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/100%,
0 170	0 070	0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-100/100%, 0-100%
0-1%	0-10%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000pppm/1%, 0-1/10%, 0-2/10%, 0-3/10%, 0-5/50%, 0-10/50%,
0 170	0.070	0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-100%, 0-100%
0-2%	0-10%	0-500/5000ppm, 0-100ppm/1%, 0-2000ppm/2%, 0-25000ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/20%, 0-5/50%, 0-10/100%,
0 270	0 10 /0	-20/100%, 0-40/100%, 0-50/100%, 0-100%, 0-100%
0-2%	0-20%	0-500/5000ppm ()-1000ppm/12%, 0-2000ppm/2%, 0-2000ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/100%,
0 270	0 20 /0	-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-3%	0-10%	0-500/5000ppm, 0-1000ppm/(2%, 0-2000ppm/2%, 0-25000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/20%, 0-5/50%, 0-10/100%,
0-370	0-1070	0-20/100%, 0-25/100%, 0-0/100%, 0-50/10%, 0-70/10%, 0-10%
0-3%	0-25%	0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-10100ppm/2%, 0-1/10%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/100%, 0-20/100%, 0-25/100%,
0-370	0-2370	0-10/10/20, 0-50/10/20, 0-70/10/20, 0-100/20, 0-50/04/01/20, 0-50/04/04/10/20, 0-50/04/20, 0-50/04/20, 0-50/10/20,
0-5%	0-25%	0-40/1003,0-0-3/0-5/,0-2/200ppm/1%,0-3000ppm/1%,0-3000ppm/1%,0-5000ppm/5%,0-1/10%,0-2/20%,0-3/25%,0-5/25%,0-10/100%,0-20/100%,0-25/100%,
0-576	0-2576	0-1000pm 1 / 8, 0-200ppm 2 / 8
0-5%	0-50%	0-1000pm/1%, 0-2000ppm/1%, 0-2000ppm/1%, 0-3000ppm/1%, 0-5000ppm/5%, 0-1/5%, 0-2/5%, 0-3/25%, 0-5/25%, 0-10/100%, 0-20/100%, 0-25/100%,
0-378	0-30 /0	0-1000phin / x, 0-200 pphin / x, 0-2000phin / x, 0-3000phin / x, 0-3000phin / x, 0-3020 x, 0-3020 x, 0-3020 x, 0-3020 x, 0-20100 x, 0-2000 x, 0
0-10%	0-50%	0-40/1003, 0-201007, 0-3/0-5/007, 0-1007, 0-1007, 0-1007, 0-1007, 0-1000, 0-20100, 0-2/10%, 0-2/10\%, 0
0-1076	0-50 %	0-1000pm1 //s, 0-200ppm1 //s, 0-200ppm1 //s, 0-3000ppm1 //s, 0-3000ppm1 //s, 0-3000ppm1 //s, 0-310/s, 0-323/s, 0-323/s, 0-320/s, 0-1030/s, 0-20100/s, 0-2000/s, 0-200
0-10%	0-100%	0-40/100%, 0-5000pm/5%, 0-1/10%, 0-5/10%, 0-5/50%, 0-10/50%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-10%	0-100%	0-3000ppm1%, 0-2010ppm1%, 0-3200ppm1%, 0-300ppm1%, 0-3000ppm1%, 0-01000ppm1%, 0-010%, 0-300%, 0-010%, 0-100/100%, 0-2010%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%, 0-2010\%,
0-20%	0-50%	0-10/00pm1/%, 0-20/0ppm1/%, 0-2000ppm1/%, 0-30/0ppm1/%, 0-30/00ppm1/%, 0-1/10%, 0-2/20%, 0-3/25\%, 0-3/25\%, 0-3/
0-25%	-	
0-40%	0-100%	0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/20%, 0-5/50%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-20%	0-100%	0-3000pp11/37%, 0-1/10%, 0-2/20%, 0-3/20%, 0-3/50%, 0-10/100%, 0-20/100%, 0-20/100%, 0-40/100%, 0-50/100%, 0-10/100%, 0-100%
0-25%	-	
0-40%	-	
	-	
0-70%		
0-100%	None	

2-component analyzer: CO₂/CH₄

1-componen		2-component: CH4
		1st range/2nd range (max.)
0-100ppm	0-1000ppm	0-500/5000ppm, 0-1000/5000ppm, 0-2000/5000ppm, 0-2500/5000ppm, 0-3000/5000ppm, 0-5000ppm
0-200ppm	0-2000ppm	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/1%, 0-5000ppm/1%, 0-1%
0-250ppm	0-2500ppm	
0-300ppm	0-2500ppm	
0-500ppm	0-2500ppm	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/2%, 0-2/10%, 0-3/10%, 0-5/10%, 0-10%
0-500ppm	0-5000ppm	0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/2%, 0-2/10%, 0-3/10%, 0-5/10%, 0-10%
0-1000ppm	0-2500ppm	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/3%, 0-1/3%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%, 0-20%
0-1000ppm	0-5000ppm	0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/3%, 0-1/3% 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%, 0-20%
0-1000ppm	0-1%	0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/3%, 0-1/3%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%, 0-20%
0-2000ppm	0-2500ppm	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%, 0-20%
0-2000ppm	0-5000ppm	0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%, 0-20%
0-2000ppm	0-2%	0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/20%, 0-20%
0-2500ppm	0-5000ppm	0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/20%, 0-5/25%, 0-10/25%, 0-20/25%, 0-25%
0-2500ppm	0-2%	0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/5%, 0-2/20%, 0-3/20%, 0-5/25%, 0-10/25%, 0-20/25%, 0-25%
0-3000ppm	0-2%	0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/5%, 0-1/5% 0-2/20%, 0-3/20%, 0-5/25%, 0-10/25%, 0-20/25%, 0-25%
0-5000ppm	0-3%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/20%, 0-5/50%, 0-10/50%,
		0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-5000ppm	0-5%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/20%, 0-5/20%, 0-10/50%,
		0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-1%	0-10%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/50%,
		0-20/50%, 0-25/50%, 0-40/50%, 0-50%
0-2%	0-20%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/10%, 0-3/10%, 0-5/25%, 0-10/100%,
		0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-2%	0-10%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/100%,
0-3%		0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-3%	0-25%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/25%, 0-10/100%,
1		0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-5%	0-20%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/100%,
		0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-5%	0-50%	0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/50%, 0-20/100%, 0-25/100%,
		0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-10%	0-20%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/100%,
		0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-10%	0-50%	0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/100%, 0-20/100%, 0-25/100%,
0-20%	/-	0-40/100%, 0-50/100%, 0-70/100%, 0-100%
0-25%	-	
0-40%	1	
0-10%	0-100%	0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/10%, 0-3/10%, 0-5/50%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%,
		0-50/100%, 0-70/100%, 0-100%
0-20%	0-100%	0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/10%, 0-3/25%, 0-5/50%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%,
0 20,0	0.0070	0-50/100%, 0-70/100%, 0-100%
0-25%	0-100%	0-2000ppm/2%, 0-2500ppm/2%, 0-3000ppm/2%, 0-5000ppm/2%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%,
0-20%	0 10070	0-20/000%, 0-20/100%, 0-100%, 0-100%
0-40 %	1	
0-50%	1	
0-100%	None	
0-10070	NUTE	

3-component analyzer: NO/SO₂/CO >>> Combination of 1st component NO and 2nd component SO₂/ 3rd component CO

1-componen	t: NO		2-componen	t: SO2	3-component: CO
1st range	2nd range (max.)		1st range	2nd range (max.)	1st range/2nd range (max.)
0-200ppm	0-2000ppm		0-200ppm	0-2000ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/2500ppm, 0-1000/2500ppm,
0-250ppm	0-2500ppm		0-250ppm	0-2500ppm	0-2000/2500ppm, 0-2500ppm
0-300ppm	0-2500ppm		0-300ppm		
0-500ppm	0-5000ppm	+	0-500ppm	0-2500ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/5000ppm, 0-1000/5000ppm,
0-1000ppm	0-5000ppm		0-1000ppm		0-2000/5000ppm, 0-5000ppm
0-2000ppm	0-5000ppm		0-2500ppm	None	
0-2500ppm	0-5000ppm		0-1000ppm	0-5000ppm	0-500/5000ppm, 0-1000/5000ppm, 0-2000/5000ppm, 0-2500/5000ppm, 0-3000/5000ppm,
0-3000ppm	0-5000ppm		0-2000ppm		0-5000ppm
0-5000ppm	None		0-2500ppm		
			0-3000ppm		
			0-5000ppm	None	

 $\label{eq:component} analyzer: CO_2/CO/CH_4 >>> Combination of 1st component CO_2/2nd component CO and 3rd component CH_4
 CH_4 >>> Combination of 1st component CO_2/2nd component CO and 3rd component CH_4
 CH_4 >>> CO_2/2nd component CO_2/2nd component CO_2/2nd component CH_4
 CH_4 >>> CO_2/2nd component CH_4
 CH_4 <br/$

1-component: CO2		2-component: CO		3-componen	t: CH4	
1st range	2nd range (max.)	1st range/2nd range (max.)		1st range	2nd range (max.)	Availability of product
0-5000ppm	0-3%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%,		0-5000ppm	0-5%	Product available only
0-1%	0-5%	0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%,				when CO analyzer max.
0-2%	0-5%	0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%				measuring range is
0-5000ppm	0-5%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/2%, 0-2500ppm/2%,	+			50% or less
		0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%,		0-1%	0-10%	Product available
		0-10/50%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%		0-2%	0-20%	
0-1%	0-10%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%,		0-3%	0-25%	Product available only
		0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/25%,		0-5%	0-10%	when CO analyzer
		0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%				measuring range is 0 to
0-2%	0-20%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%,		0-10%	0-20%	1000ppm or more.
		0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%,		0-20%	0-25%	Product available only
		0-10/50%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%		0-25%	0-40%	when CO analyzer
0-2%	0-10%	0-500/5000ppm, 0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%,		0-25%		measuring range is 0 to
0-3%	0-25%	0-3000ppm/2%, 0-5000ppm/5%, 0-1/10%, 0-2/20%,0-3/25%, 0-5/50%,		0-40%	0-50%	5000ppm or more.
0-5%	0-50%	0-10/100%, 0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%				Available only when
0-10%	0-100%	0-1000ppm/1%, 0-2000ppm/1%, 0-2500ppm/1%, 0-3000ppm/2%,		0-50%	0-70%	the CO analyzer range
0-20%		0-5000ppm/5%, 0-1/10%, 0-2/20%, 0-3/25%, 0-5/50%, 0-10/100%,		0.700/	0.1000/	is 0–5000 ppm or more,
0-25%		0-20/100%, 0-25/100%, 0-40/100%, 0-50/100%, 0-70/100%, 0-100%		0-70%	0-100%	and the CO ₂ analyzer
0-40%]			0-100%	None	range is 0–2% or more
0-50%]			0-10070	NULLE	
0-70%						
0-100%	None					

 $\label{eq:component} 4-component analyzer: NO/SO_2/CO_2/CO >>> \quad Combination of 1st component NO/4th component CO and component SO_2/3rd component CO_2 and component SO_2/3rd component CO_2 and component SO_2/3rd compone$

1-component: NO		4-component: CO
1st range	2nd range (max.)	1st range/2nd range (max.)
0-200ppm	0-1000ppm	
0-250ppm	0-1000ppm	
0-300ppm	0-1000ppm	0.000/0000
0-500ppm	0-2000ppm	0-200/2000ppm, 0-250/2500ppm, 0-300/2500ppm, 0-500/2500ppm, 0-1000/2500ppm, 0-2000/2500ppm, 0-2500ppm, None
0-1000ppm	0-2000ppm	
0-2000ppm	None	
0-500ppm	0-5000ppm	
0-1000ppm	0-5000ppm	
0-2000ppm	0-5000ppm	0-500/2500ppm, 0-1000/2500ppm, 0-2000/2500ppm, 0-2500ppm, None
0-2500ppm	0-5000ppm	0-300/2300ppm, 0-1000/2300ppm, 0-2000/2300ppm, 0-2300ppm, None
0-3000ppm	0-5000ppm	
0-5000ppm	None	
-	F	


2-component analyzer: SO2		3-component analyzer: CO ₂		
1st range	2nd range (max.)	1st range/2nd range (max.)		
0-200ppm	0-2000ppm			
0-250ppm	0-2500ppm			
0-300ppm	0-2500ppm			
0-500ppm	0-5000ppm			
0-1000ppm	0-5000ppm	0-1/10%, 0-2/20%, 0-3/20%, 0-5/50%, 0-10/50%, 0-20/50%, 0-25/50%, 0-40/50%, 0-50%/None		
0-2000ppm	0-5000ppm			
0-2500ppm	0-5000ppm			
0-3000ppm	0-5000ppm			
0-5000ppm	None			

Code sym		04-1-11-11	Diselection to contract
6th digit	7th digit	21st digit	
Y	1 to 4, D	Y	Ch1:O2
Р	Y	Y	Ch1:NO
A	Y	Y	Ch1:SO ₂
D	Y	Y	Ch1:CO ₂
В	Y	Y	Ch1:CO
E	Y	Y	Ch1:CH4
F	Y	Y	Ch1:NO, Ch2:SO2
G	Y	Y	Ch1:NO, Ch2:CO
Н	Y	Y	Ch1:SO ₂ , Ch2:CO ₂
J	Y	Y	Ch1:CO ₂ , Ch2:CO
K	Y	Y	Ch1:CH4, Ch2:CO
L	Y	Y	Ch1:CO ₂ , Ch2:CH ₄
Ν	Y	Y	Ch1:NO, Ch2:SO ₂ , Ch3:CO
Т	Y	Y	Ch1:CO ₂ , Ch2:CO, Ch3:CH ₄
V	Y	Y	Ch1:NO, Ch2:SO ₂ , Ch3:CO ₂ , Ch4:CO
Р	1 to 4, D	Y	Ch1:NO, Ch2:O2
А	1 to 4, D	Y	Ch1:SO ₂ , Ch2:O ₂
D	1 to 4, D	Y	Ch1:CO ₂ , Ch2:O ₂
В	1 to 4, D	Y	Ch1:CO, Ch2:O2
E	1 to 4, D	Y	Ch1:CH4, Ch2:O2
F	1 to 4, D	Ý	Ch1:NO, Ch2:SO ₂ , Ch3:O ₂
G	1 to 4, D	Ý	Ch1:NO, Ch2:CO, Ch3:O2
H	1 to 4, D	Y	Ch1:SO ₂ , Ch2:CO ₂ , Ch3:O ₂
J	1 to 4, D	Y	Ch1:CO ₂ , Ch2:CO ₂ , Ch3:O ₂
K	1 to 4, D	Y	Ch1:CH ₄ , Ch2:CO, Ch3:O ₂
L	1 to 4, D	Y	Ch1:CO ₂ , Ch2:CH ₄ , Ch3:O ₂
 N	1 to 4, D	Y	Ch1:NO, Ch2:SO ₂ , Ch3:CO, Ch4:O ₂
T	1 to 4, D	Y*	Ch1:CO ₂ , Ch2:CO, Ch3:CH ₄ , Ch4:O ₂
V	1 to 4, D	Y*	Ch1:NO, Ch2:SO ₂ , Ch3:CO ₂ , Ch4:CO, Ch5:O ₂
 P			
	1 to 4, D	A *	Ch1:NOx, Ch2:O2, Ch3:corrected NOx
A	1 to 4, D	A *	Ch1:SO ₂ , Ch2:O ₂ , Ch3:corrected SO ₂
В	1 to 4, D	A *	Ch1:CO, Ch2:O ₂ , Ch3:corrected CO
F	1 to 4, D	A *	Ch1:NOx, Ch2:SO ₂ , Ch3:O ₂ , Ch4:corrected NOx, Ch5:corrected SO ₂
G	1 to 4, D	A *	Ch1:NOx, Ch2:CO, Ch3:O ₂ , Ch4:corrected NOx, Ch5:corrected CO
J	1 to 4, D	A *	Ch1:CO ₂ , Ch2:CO, Ch3:O ₂ , Ch4:corrected CO
N	1 to 4, D	A *	Ch1:NOx, Ch2:SO ₂ , Ch3:CO, Ch4:O ₂ , Ch5:corrected NOx, Ch6:corrected SO ₂ , Ch7:corrected CO
V	1 to 4, D	A *	Ch1:NOx, Ch2:SO ₂ , Ch3:CO ₂ , Ch4:CO, Ch5:O ₂ , Ch6:corrected NOx, Ch7:corrected SO ₂ , Ch8:corrected CO
Р	1 to 4, D	C *	Ch1:NOx, Ch2:O ₂ , Ch3:corrected NOx, Ch4:corrected NOx average
Α	1 to 4, D	C *	Ch1:SO ₂ , Ch2:O ₂ , Ch3:corrected SO ₂ , Ch4:corrected SO ₂ average
В	1 to 4, D	С	Ch1:CO, Ch2:O ₂ , Ch3:corrected CO, Ch4corrected CO average
F	1 to 4, D	C *	Ch1:NOx, Ch2:SO ₂ , Ch3:O ₂ , Ch4:corrected NOx, Ch5:corrected SO ₂ , Ch6:corrected NOx average,
			Ch7:corrected SO ₂ average
G	1 to 4, D	C *	Ch1:NOx, Ch2:CO, Ch3:O ₂ , Ch4:corrected NOx, Ch5:corrected CO, Ch6:corrected NOx average,
		*	Ch7:corrected CO average
J	1 to 4, D	С	Ch1:CO2, Ch2:CO, Ch3:O2, Ch4:corrected CO, Ch5:corrected CO average
Ν	1 to 4, D	C *	Ch1:NOx, Ch2:SO ₂ , Ch3:CO, Ch4:O ₂ , Ch5:corrected NOx, Ch6:corrected SO ₂ , Ch7:corrected CO,
			Ch8:corrected NOx average, Ch9:corrected SO2 average, Ch10:corrected CO average
V	1 to 4, D	С	Ch1:NOx, Ch2:SO2, Ch3:CO2, Ch4:CO, Ch5:O2, Ch6:corrected NOx, Ch7:corrected SO2, Ch8:corrected CO
			Ch9:corrected NOx average, Ch10:corrected SO2 average2, Ch11:corrected CO average

Table 2 Channel (Ch) No. and display/output contents comparison table

 * When the 21st digit code is A or C, the component of the NO analyzer is displayed as NOx.

DIMENSIONS (Unit : mm)

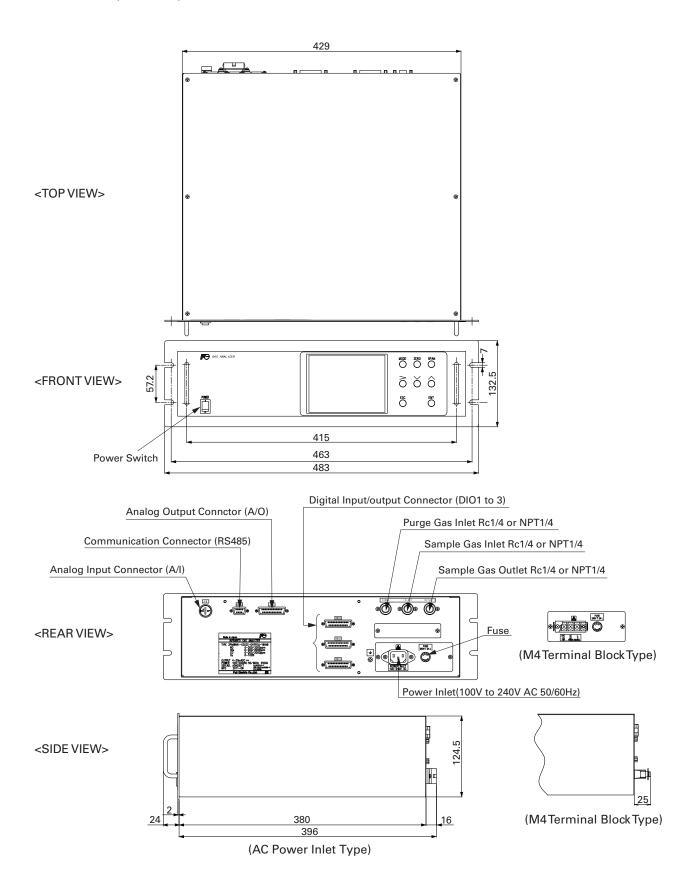


14


Mounting method


The analyzer weight should be supported at the bottom of the case.

19-inch rack mounting type










EXTERNAL CONNECTION


<Analog output> A/O connector



D-sub 25pins female

* In standard, displayed Channel No. and Analog Output No. are same.

<Screw terminal (M4)>







1	A01+
14	A01-
2	A02+
(15)	A02-
3	A03+
16	A03-
4	A04+
(17)	AO4-
5	A05+
18	
6	A06+
19	
0	A07+
@	A07-
8	A08+
2)	A08-
9	AO9+
	A09-
10	AO10+
23	AO10-
1)	A011+
24	A011-
12	AO12+
25	AO12-
13	NC

SCOPE OF DELIVERY


- Gas analyzer ... 1 unit
- Replacement fuse (250V AC, 2A, delay type) ... 2 pcs
- Instruction manual ... 1 copy
- Connector for I/O connection ... 1 set
- When the 4th code is "D": power supply cord (standard inlet type 2m) ... 1 pc

ORDERING INFORMATION

1. Code symbols

2. Application and composition of sample gas

<RS485 communication signal>



<Analog input> A/I connector (O2 signal input)

Al-

<Digital I/O> DIO 1 to 3 connector (option)

DI3 DI4 DI5 DI6

DI7

DI8

DI9

<digita< th=""><th>al I/O> DIO 1 to 3</th><th>conr</th><th>necto</th><th>or (</th><th>opti</th><th colspan="4">DIO1 DIO2 DIO3</th></digita<>	al I/O> DIO 1 to 3	conr	necto	or (opti	DIO1 DIO2 DIO3											
13		1								connector	connector	r connector					
0	000000000000000000000000000000000000000	0								DI1+ DI1-	DI4+ DI4–	DI7+ DI7-	Disital is sut				
2	5 14	1						, —	-2	DI2+	DI5+	DI8+	Digital input OFF: 0V				
_								r		DI2-	DI5-	DI8-	ON : 12 to 24V DC				
D	-sub 25pins femal	е						<u>ہ</u>	-3	DI3+	DI6+	DI9+					
* DI	O 1 to 3 are all sa	ma t	wno	of	onr	hort	or			DI3-	DI6-	DI9– J	J				
		ne t	ype	010	.0111	1001	51.	٢		D01	DO6	DO11))				
								o	-5 NO								
Conter	nts of digital input	sigr	nal					۶									
DI1	Remote hold]						\o		DO2	D07	DO12					
DI2	Average value reset							°	19 NO ↓ ⑦ NC ∖				Contact capacity				
DI3	A. cal. start]						٢	@ com }	DO3	DO8	DO13	24V DC/1A				
DI4	A. zero. cal. start							o	-8 NO	200	200	20.0					
DI5	Remote range Ch1							6									
DI6	Remote range Ch2							6	—⑨com	DO4	DO9	DO14					
DI7	Remote range Ch3	-						o	—2 NO J								
DI8	Remote range Ch4	-						<u>م</u>	10 NC 	DO5	DO10	DO15					
DI9	Remote range Ch5							°		005	DOTO	0015)					
									@								
Allocation table of digital input signal									12								
22th dig	git→ A B C D	E	F	G	Н	Y			_25								
DI1			9		$ \circ\rangle$				13								
DI2		$ \bigcirc$	$ \circ $	0	O												

 \odot sign shows the function is valid.

)*

0*

()*

0*

⊜*

_>*

0*

0*

)*)*

<u>}*</u>

)*

)*)*

)*

* : The function might be invalid depending on the number of measurable components.

For example: DI5 corresponds to 1st component, DI6 corresponds to 2nd components.

Contents of digital output signal

number of com-	e											
number of compor	· I-component an					2-component analyzer		3-component analyzer				
A, C	В, Е		D, F, G, H		B, D, E, F, G, H		B, D, E, F, G, H					
Instrument error		Instrument erro	or Instrument erro		r	Instrument error		Instrument error				
Calibration error	error Calibration			Calibration error		Calibration error		Calibration error		T I		
		A.cal.status	(A.cal.status)			(A.cal.status)		(A.cal.status)		1		
		For zero gas	(For zero gas)			(For zero gas)		(For zero gas)		, ,		
		For span gas Ch1		1 (For span gas Ch		 (For span gas Ch1) 		(For span gas Ch1)		0	/ 1	e 011
(Alarm1)		(Alarm1)				(For span gas Ch2)		(For span gas Ch2)				
(Alarm2)		(Alarm2)						(For span gas Ch3)		The normal open side (NO) of digital output is close when the function is active without range ID.		
(Alarm3)		(Alarm3)						(Range identification Ch1)				
(Alarm4)		(Alarm4)				(Range identification Ch1)		(Range identification Ch2)				
(Alarm5)		(Alarm5)		Range identification		(Range identification Ch2)		(Range identification Ch3)				
				(Alarm1)		(Alarm1)		(Alarm1)				
				(Alarm2)		(Alarm2)		(Alarm2)				
				(Alarm3)		(Alarm3)		(Alarm3)			. ,	vvicii
				(Alarm4)		(Alarm4)		(Alarm4)		The normal close (NC) side is		
			(Alarm5)			(Alarm5)		(Alarm5)		close with Second range.		
4 component anal							Eaam					
			G H						<i>.</i>		G	
· ·	<i>'</i>	, 		-				montorror	- / ·	orror		
		-										
	Campration error											
-			-			5		-			-	
										ation Ch1	· · · ·	
	Panga identification Ch1							-	-			
			i oi spail gas cil4					-				
					l .	0		an gas cho	-			
	°				·						Bange identification Ch1	
	,		Bange identification Ch1									
	(Alarm3)		Range identification Ch2			(Alarm3)		(Alarm2) (Alarm3) (Alarm3			Range identification Ch3	
	Mall			Range identification Ch3		(Alarms) Range identification Ch3					mange lucilumation Cha	
(Alarm4)	· · · ·	m4)	Rang	e identification Ch3	Bang	e identification Ch?	(Alarn	n4)	(Alarm4)		Range identification Ch4	
	A, C Instrument error Calibration error (Alarm1) (Alarm2) (Alarm3) (Alarm3) (Alarm4) (Alarm5) 4-component anal- B, E Instrument error Calibration error A.cal.status For zero gas For span gas Ch2 For span gas Ch2 For span gas Ch3	A, C Instrument error Calibration error (Alarm1) (Alarm2) (Alarm3) (Alarm4) (Alarm5) 4-component analyzer B, E D, F Instrument error B, E D, F Instrument error Calibration error Calibration error Calibration error Calibration error Calibration error Calibration error Calibration error Calibration error Calibration error For span gas Ch1 For span gas Ch2 For span gas Ch3 Range Range Range (Alarm1) (Alarm1) (Alarm1) (Alarm1) (Alarm1)	A, C B, E Instrument error Instrument error Calibration error Calibration error A.cal.status For zero gas For span gas C (Alarm1) (Alarm2) (Alarm3) (Alarm3) (Alarm3) (Alarm3) (Alarm4) (Alarm4) (Alarm5) (Alarm5) A.cal.status For span gas Ch B, E D, F Instrument error Calibration error A.cal.status For span gas Ch1 For span gas Ch2 For span gas Ch2 Range identification Ch2 Range identification Ch4 (Alarm1) (Alarm1)	A, C B, E Instrument error Instrument error Calibration error Calibration error A.cal.status For zero gas For span gas Ch1 (Alarm1) (Alarm2) (Alarm3) (Alarm3) (Alarm3) (Alarm3) (Alarm4) (Alarm3) (Alarm4) (Alarm3) (Alarm5) (Alarm3) (Alarm5) (Alarm5) 4-component analyzer B, E D, F G Instrument error Instrument error Instr Calibration error Calibration error Calif A.cal.status A.ca For span gas Ch1 For span gas Ch2 Range identification Ch3 For span gas Ch4 Range identification Ch3 Range identification Ch4 (Alarm1) (Alarm1) (Alarm1) (Alarm1)	A, C B, E D, F, G, H Instrument error Instrument error Calibration	A, CB, ED, F, G, HInstrument errorInstrument errorInstrument errorCalibration error(Alarm1)(Alarm1)(Acal.status)(Alarm2)(Alarm2)(Alarm3)(Alarm3)(Alarm3)(Alarm1)(Alarm5)(Alarm4)(Alarm2)(Alarm5)(Alarm5)Range identification Ch1(Alarm5)(Alarm5)Range identification Ch1(Alarm4)(Alarm5)Range identification Ch1(Alarm5)(Alarm4)(Alarm3)(Alarm4)(Alarm4)(Alarm4)(Alarm5)(Alarm4)(Alarm4)(Alarm4)(Alarm4)(Alarm5)4-component analyzerInstrument errorB, ED, FGHInstrument errorInstrument errorCalibration errorFor span gas Ch1<	A, C B, E D, F, G, H B, D, E, F, G, H Instrument error Instrument error Instrument error Instrument error Calibration error Calibration error Calibration error Calibration error Calibration error Calibration error Calibration error Calibration error A.cal.status (A.cal.status) (A.cal.status) (A.cal.status) For zero gas (For zero gas) (For span gas Ch1) (For span gas Ch2) (Alarm1) (Alarm2) (Alarm2) (Alarm3) (Alarm3) (Alarm3) (Range identification Ch1) (Range identification Ch1) (Alarm5) (Alarm4) (Alarm2) (Alarm2) (Alarm5) (Alarm3) (Alarm2) (Alarm2) (Alarm4) (Alarm3) (Alarm3) (Alarm3) (Alarm5) (Alarm3) (Alarm3) (Alarm3) (Alarm4) (Alarm3) (Alarm3) (Alarm3) (Alarm5) (Alarm4) (Alarm3) (Alarm3) (Alarm5) (Alarm5) (Alarm5) (Alarm3) (Alarm5) (Alarm5) (Alarm5) (Alarm5)	A, C B, E D, F, G, H B, D, E, F, G, H Instrument error Instrument error Instrument error Instrument error Calibration error Calibration error Calibration error Calibration error (Alarm1) (Alarm1) (For span gas Ch1) (For span gas Ch2) (Alarm2) (Alarm2) (Alarm3) (Alarm3) (Alarm4) (Alarm5) Range identification Ch1 (Range identification Ch2) (Alarm5) (Alarm5) (Alarm3) (Alarm3) (Alarm3) (Alarm5) (Alarm3) (Alarm3) (Alarm3) (Alarm4) (Alarm3) (Alarm4) (Alarm4) (Alarm5) (Alarm5) (Alarm5) (Alarm4) (Alarm5) (Alarm5) (Alarm5) S-conr <td< td=""><td>A, CB, ED, F, G, HB, D, E, F, G, HB, C, E, Calibration errorCalibration errorCalibrati</td><td>Instrument errorInstrument errorInstrument errorInstrument errorInstrument errorInstrument errorInstrument errorInstrument errorInstrument errorCalibration errorCalibratio</td><td>A, C B, E D, F, G, H B, D, E, F, G, H B, D, E, F, G, H B, D, E, F, G, H Instrument error Instrument error Instrument error Instrument error Calibration error Caligitation error Calibration error</td></td<> <td>A, C B, E D, F, G, H B, D, E, F, G, H Calibration error Calibration error<</td>	A, CB, ED, F, G, HB, D, E, F, G, HB, C, E, Calibration errorCalibration errorCalibrati	Instrument errorInstrument errorInstrument errorInstrument errorInstrument errorInstrument errorInstrument errorInstrument errorInstrument errorCalibration errorCalibratio	A, C B, E D, F, G, H B, D, E, F, G, H B, D, E, F, G, H B, D, E, F, G, H Instrument error Instrument error Instrument error Instrument error Calibration error Caligitation error Calibration error	A, C B, E D, F, G, H B, D, E, F, G, H Calibration error Calibration error<

Zirconia O₂ analyzer (to be purchased separately)

Measuring method:

Zirconia system

Measurable component and measuring range:

	Measurable	e component	Range					
	O2	Oxygen	0 to 25vol%					
Re	peatability:	Within $\pm 0.5\%$ of full scale						
Lin	earity:	Within ± 1% of full scale						
Zei	ro drift:	Within ± 1% of full scale/week						
Sp	an drift:	Within ± 2% of full scale/week						
Re	sponse time:	Approx. 20 seconds (for 90% response)						
Measured gas flow rate:								

0.5 ± 0.25L / min

Notes:

- If process gas is combustible, measurement error may occur due to oxygen contained in the process gas.
- If process gas is corrosive (for example, SO₂ beyond 250 ppm range), the service life of zirconia sensor may be shortened.


Gas inlet/outlet size:


Rc1/4 or NPT1/4

DIMENSIONS (Unit: mm)

 Power supply: Rated voltage; 100 to 115V AC or 200 to 240V AC Rated frequency; 50Hz/60Hz Max. rated power; 215VA (at start up) 65VA (during normal operation)
 Enclosure: Steel casing, for indoor application Indication: Temperature indication (LED)
 Temperature alarm output: Contact output 1 from A contact, Contact capacity 220V AC, 1A (resistive load)
 Outer dimensions (H x W x D): 141 x 170 x 190mm
 Weight: Approx. 3kg
 Finish color: Munsell 5Y 7/1

CODE SYMBOLS

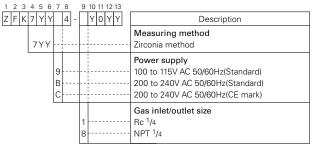

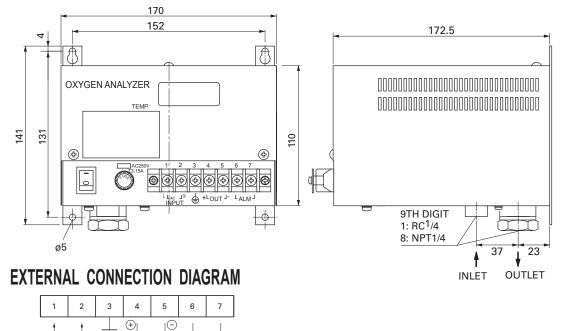

Information in this catalog is subject to change without notice. Read the instruction manuals thoroughly before using the products.

Output

to ZPA

F Fuji Electric Co., Ltd.

Е

AC power supply

Gate City Ohsaki, East Tower, 11-2, Osaki 1-chome, Shinagawa-ku, Tokyo 141-0032, Japan Phone: +81-3-5435-7111 www.fujielectric.com www.fujielectric.com/products/sensors_measurements/instruments/index.html

Temperature

alarm output